





93-531 Łódź



ignis 160 solis 160 solis 60 solis 30 medivent

new technologies in good light



Famed Łódź history dates back to pre-WWII times, when as Elektrosan, the company manufactured medical equipment, among others for the Military Hospital in Łódź. The trading name has changed since, but the business has remained the same.

State-Owned FAMED-1 Electromedical Equipment Factory was the legal successor of State-Owned Electrical Equipment Factory in £ódz established with an ordinance of the Minister of Heavy Industry on 31 December 1949, then transformed a number of times. Initially, the factory was housed in the office and manufacturing premises given to the company in the centre of Łódź, at 6 Komuny Paryskiej Square. In 1968 the enterprise moved to the new facilities at 2 Szparagowa Street. Fabryka Aparatury Elektromedycznej FAMED Łódź S.A. was established as a result of commercialization of FAE FAMED-1 state-owned company carried out by the Minister of Treasury on 23 April 1998. In 2010 the company was privatised and added to the ORGANIKA Group. During the restructurisation process, the offices of the company were moved to 21a Ciasna Street in 2011.

### about us







Our products meet the requirements of the European Directive MDD 93/42/EEC and European standards IEC 60601-1:2011, IEC 60601-1-2:2007.

#### AC090 MD/1463/4450/2016

Currently Famed Łódź is reputable Polish manufacturer of lighting systems. In our assortment we have got OT and examination lights, as well as diagnostic and UV sterilization lamps intended for use indoctor's offices.

Lamps manufactured by Famed use conventional halogen bulbs as the light source, as well as LEDs, which offer longer service life, high light intensity and electricity savings. In addition, LED operating lights enable switching on green LEDs only, which is convenient for endoscopic procedures (highest haemoglobin absorption occurs at a wavelength corresponding to green colour so that no reflections are generated with the green light that would hinder interpretation of the endoscopic image).

We are a manufacturer of high quality medical equipment renowned in Poland and abroad. Our longtime presence in the medical industry and the experience gained in connection with the use of modern technologies guarantee the high quality of our products. We are able to adapt to the individual needs of each customer in terms of the equipment, which makes our products tailored to the needs of our customers. We provide high quality products, professional service and professional advice - in accordance with ISO 9001:2008 and ISO 13485:2012 quality assurance systems.

NEW TECHNOLOGIES IN GOOD LIGHT is our mission that we pursue in order to fully meet your expectations.

1939

1950

1970

1980

1990


2010

2014

2015

Establishment of the company

Beginning of mass production of medical lamps Production of lamps with halogen hulbs SURGILUX Production of lamps with halogen bulbs SURGILUX Introduction of examination halogen lamps MEDILUX Implementation of LED lamps LEDILUX. Introduction of a family of LED lamps SOLIS Introduction of LED lamps IGNIS

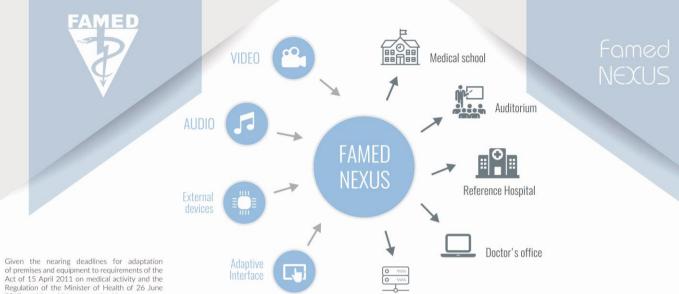

Regulation of the Minister of Health of 26 June 2012, entities which operate health care centres have been engaged in intensive modernization work, also in operating rooms.

If you carry out work related to adaptation of operating rooms to statutory requirements, it is worth thinking about fitting out the operating room with surgery recording solutions. The draft amendment of the Act of 2011 on the system of information in the health care sector assumes that after 31 December 2017 all entities which provide medical services will be obliged to keep individual medical records in the electronic form only.

Digital recording of the surgery progress is an essential function that supports retrieval of the material in the event of any claims brought by the patient. Currently with the increasing number of claims brought by patients and activities of legal firms which specialize in claiming of damages, it may turn out that an investment in such a system will break even very soon. Besides recording the surgery progress, a properly developed system may support communication and image transmission from the operating rooms and medical imaging equipment (endoscope, laparoscope, C-arm) to remote locations, such as lecture rooms, doctor's surgeries or other medical centres. The use of audio-visual modules supports transmission of data from information systems, remote medical consultations or archiving of materials for training purposes. Solutions that we offer are designed in cooperation with our partner who has years of experience in development of audio-visual systems used in operating rooms.

### Archiving device





Medical tablets support remote control of video and audio coming from various medical devices. These are high quality devices, resistant to dirt and mechanical damage.



wall-mounted control panel

A control panel gives you remote, wired access to the operating light functions. As it is wall-mounted, any change in light intensity, colour temperature or camera zoom is even easier and reachable without entering the surgeon's working zone.



recorder

Medical recorders perfectly complement operating lights with in-built cameras. Support for recording hundreds of Full HD video guarantees protection of hospital's sensitive data. The video can be shared real-time for teaching purposes.



open architecture

Open architecture supports customization of an integrated system to the hospital's needs. This combination of information technology with advanced medical technology guarantees the highest level of medical services.

services.
The entire solution
is covered with secure glass that
ensures easy disinfection and
constant camera and light
parameters.

## ignis 160

















The control panel – the possibility to control light and camera parameters, using only one control panel. The dome has two identical control panels, which makes it simple to steer the lamp parameters independently of the location of the dome.





The construction guarantees easiness of use and cleaning.

By applying a small amount of external elements the dome is well protected against water and dust. Two handles — the sterile handle allows focusing of the light spot. The non-sterile handle surrounds the dome in more than 75% of its circumference, which provides independent access and makes the positioning very easy. The unique solution are two control panels located on the dome opposite each other, which provides a good access independently of the position of the operator.

Additionally, these panels allow to control not only the parameters of the light but also the parameters of the image (option with the HD camera).

**IGNIS 160** is equipped with an independent option of green light for the endoscope procedures. Thanks to our 75 years of experience, we've been able to equip the lamp with a function of the additional illumination of the surgical field, effective even in cases of the deepest operating fields.

Lighthead	IGNIS 160
Supply voltage	24 V DC
Light intensity at a distance of 1 m (Ec)	160 000 lux
Adjustable light intensity	25 + 100%
Colour rendering index Ra	96
Colour temperature	4000 / 4400 / 4800 8
Operating field diameter d10	280 mm
Light spot diameter d50	140 mm
Adjustable diameter of the operating field	yes
Temperature increase near surgeon's head	<1°C
Depth of illumination L1+L2	140 cm
Power consumption for the lighthead	50 W
Insulation class	1
Protection degree provided by lighthead enclosure	IP 54









The control panel – easy to use, with the turn on/off button and adjustment of the light intensity.

The sterile handle – enables focusing of the light spot of the operating field, ergonomic, placed in the center for easy access and positioning of the dome.

Domes – three separated light sources, in the case of failure of one of them, the other two sources provide adequate illumination. The dome doesn't have any external screws and other fasteners. The smooth surface and perfectly matched components, guarantee keeping it perfectly (etan.

Construction and properties of operating and surgery lights as well as surgery sets SOLIS 160 ensure meeting of all requirements with respect to the illumination of operating/surgery field, binding for the equipment of this kind. A new construction of lightheads consists in the application of a "slim" version of the projector enclosure, characterized by a high protection degree (IP 43).

Lighthead	SOLIS 160
Supply voltage	24V DC
Light intensity at a distance of 1 m (Ec)	160 000 lx
Adjustable light intensity	25 ÷ 100%
Colour rendering index Ra	96
Colour temperature	4400 K
Operating field diameter d10	210 mm
Light spot diameter d50	110 mm
Adjustable diameter of the operating field	yes
Temperature increase near surgeon's head	<1°C
Depth of illumination L1+L2	50 cm
Power consumption for the lighthead	50 W
Insulation class	1
Protection degree provided by lighthead enclosure	IP 43






Movements are possible thanks to the sterilizable handle. The ergonomic design guarantees a high handling and the versions available allow use in any surgery or laboratory.

The arm moves vertically thanks to a spring-compensated balancing system, has a side full-circle handling without any With innovative "no touch" control light intensity can be adjusted to your personal at a distance of 1 m) and the technical performance suit a lamp for precision operations, in intensive care, recovery room and first aid station; its handy and nonbulky structure makes it suitable for diagnostic use, pre-operating theatres and test laboratories as well. With innovative "no touch" control light intensity can be adjusted to your personal needs.

Lighthead	SOLIS 60
Supply voltage	24V DC
Light intensity at a distance of 1 m (Ec)	60 000 lx
Adjustable light intensity	50 ÷ 100% touchless
Colour rendering index Ra	96
Colour temperature	4400 K
Operating field diameter d10	220 mm
Light spot diameter d50	110 mm
Adjustable diameter of the operating field	no no
Temperature increase near surgeon's head	<1°C
Depth of illumination L1+L2	130 cm
Power consumption for the lighthead	19 W
Insulation class	1
Protection degree provided by lighthead enclosure	IP 43

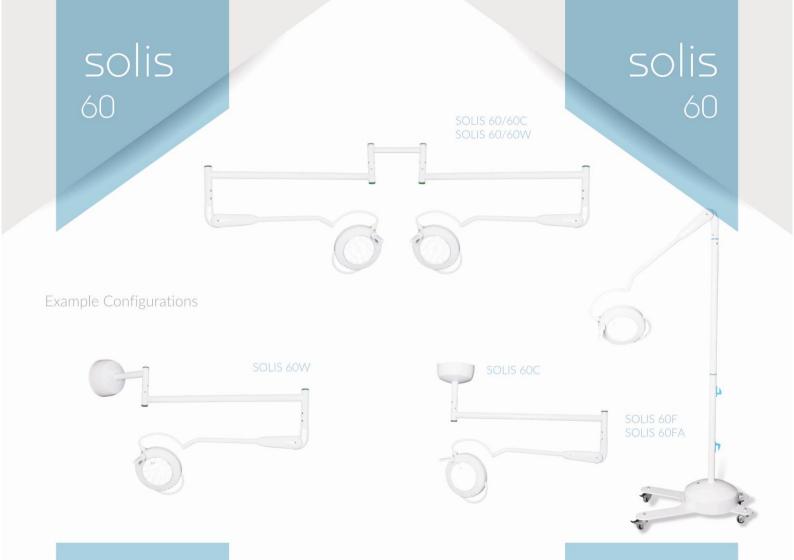

# solis





SOLIS 30C SOLIS 30M

Example Configurations



## solis 30



Rail mounted version.



Ergonomic handle let you easily adjust the light.



Goosneck arm highly increases the manoeuwability of the lamp.



Lights intensity can be adjusted fluently beetwen 15-100%


Wherever you need to conduct a clinical exam SOUS 30 will be at your side to guarantee optimal lighting in all situations. SOUIS 30 light delivers 30 000 lux at 1 m, providing ideal illumination for all medical specialities. With faithful colour mendering (CRI 96), the SOUIS 30 is particularly well suited for demantalogy. The use of FLDs ensures that the light does not give off heat. With rail-mounted, mobile, ceiling and wall versions available, SOUIS 30 is suitable for all work environments. To make practitioners' everyday tasks easier and avoid maintenance problems, the SOUIS 30 uses IEDs which have a considerably longer service life than halogen bulbs, leaving practitioners free to devote all their time to patients. The round and utur-flat shape of the fight makes the product ergonomic and suitable for any type of installation. Smooth and rounded shape of the dome make it easy to clean and disinfect. The road aid layout of the lenses and lamp diameter permit shadow suppression and three-dimensional lighthiq.

Lighthead	SOLIS 30	
Supply voltage	24V DC	
Light intensity at a distance of 1 m (Ec)	30 000 lx	
Adjustable light intensity	15 ÷ 100%	
Colour rendering index Ra	96	
Colour temperature	4400 K	
Operating field diameter d10	210 mm	
Light spot diameter d50	105 mm	
Adjustable diameter of the operating field	no	
Temperature increase near surgeon's head	<1°C	
Depth of illumination L1+L2	100 cm	
Power consumption for the lighthead	12 W	
Insulation class	1	
Protection degree provided by lighthead enclosure	IP 43	





- WALL MOUNTED •
- CEILING MOUNTED •
- MOBILE VERSION •













## medivent





Influenza

### BACTERIA

Legionolla pnoumophila Staphylococcus aureus Bacillus megatherium Bacillus megatherium spores Streptooccus haemulyticus Bacillus antharacis Corynebacterium diphtheriae Pseudomonas aerueinosa

Bacillus tuberculosis

### VIRUSES FUN Pelievirus Saccha Infectious hepatitis Saccha

Saccharonyces corevisiae
Saccharonyces spores
Aspengillus flavus
Aspengillus niger
Mucer racemedus
Penicillium digitatum
Rhizapus nigricans
Cladesporium herbarum